
S.U.P.A.™ Slide Instructions

MPC	Description	Dimensions
REF		
LOCO-200	Standard	200cm x 75cm
LOCO-555	Medium	200cm x 85cm
LOCO-201	Wide	200cm x 100cm



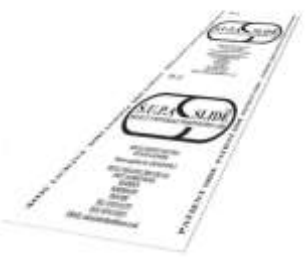

⚠ All patient moving and handling tasks should be carried out in accordance with approved patient moving and handling techniques and after a full assessment of patient, equipment, task and environment. Always follow the approved policy of your place of work when adopting moving and handling practices.

Description


The Locomotor S.U.P.A. (Select Universal Positioning Aid) Slide is a disposable / single patient use slide sheet available in standard, medium and wide sizes.
The S.U.P.A. Slide can be used either in pairs or singularly to reposition or transfer a patient in conjunction with a bed, trolley, theatre table, examination couch or similar. S.U.P.A. Slides are delivered in a dispensing box of 100 sheets.

Instructions for use

⚠ Always ensure that any part of the patient not assisting with the transfer is on two layers of slide sheet.

Open the dispensing box as per instructions printed on the box and remove the required number of sheets.

Used in pairs:

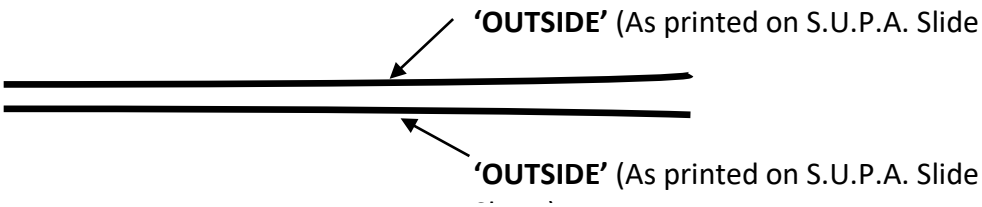


- Place one S.U.P.A Slide on top of another ensuring that the repeatedly printed instruction 'OUTSIDE' is on the outside of each S.U.P.A. Slide.
- Using an approved manual handling technique roll the patient and insert the sheets underneath the patient. Ensure that any part of the patient that is not assisting with the transfer is on two layers of S.U.P.A. Slide.

Instructions for use (continued)

- To perform a transfer, take hold of the top S.U.P.A. Slide and slide the patient to the required position.
- The S.U.P.A. Slide can then be removed by folding a corner of each sheet back underneath itself and sliding one layer against the other until free of the patient. Steady the patient as the S.U.P.A. Slide is removed.

Used singularly:

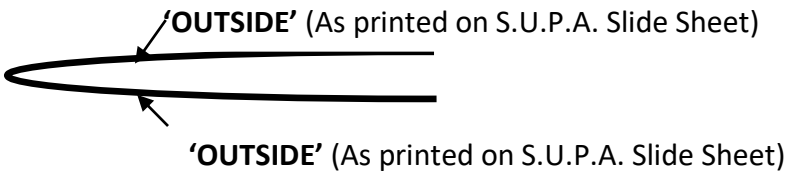

- Fold the S.U.P.A. Slide to form a loop (open tube), ensuring that the printed instruction 'OUTSIDE' is on the outside.
- Roll the patient and insert in the desired position. Ensure that any part of the patient that is not assisting with the transfer is on two layers of S.U.P.A. Slide.
- To perform a transfer take hold of the top layer of the S.U.P.A. Slide and slide the patient to the required position. The S.U.P.A. Slide can then be removed by folding a corner of the sheet back underneath itself and sliding one layer against the other until free of the patient. Steady that patient as the S.U.P.A. Slide is removed.

⚠ **For further information and training on moving and handling techniques please contact your Moving and Handling Advisor or similar**.

Care and use

⚠ **Inspect before each use. Do not use if damaged or soiled.**

Single patient use (patient specific)

Do not launder

Storage

Store away from sunlight and sources of heat

Store in dry conditions

Specifications

Material: Spun bonded, non-woven, silicone coated polypropylene

Latex free

Maximum user weight (MUW): 200 kg

Not for lifting

Disposal

May be recycled where facilities exist

Soiled waste to be delt with according to your organisations policy and procedures

---

Warranty

Warranted to specification for 12 months from date of purchase.

Applied regulations and standards

MD Class 1 Medical Device UK MDR 2002 EU MDR 2017/745 BS EN 12182: 2012 Tech Aids for disabled persons	CE UKCA

For further assistance please contact your supplier or customer services at:

Manufacturer

Select Healthcare (UK) Ltd.
Unit 2 Albert Road
Rushden
Northants
NN10 0BU

Tel: +44 (0) 1933 411729
Fax +44 (0) 1933 410213
Email: info@selecthealthcare.co.uk
Website:
www.selecthealthcare.co.uk

European Representative

EC REP **Select Healthcare (EU),** 72 Liffock Park, Coleraine, Northern Ireland, BT51 4DG

Glossary of symbols and terms used in product and packaging labels that are not expressed above.

Symbol	Meaning	Associated Terms
	Consult instructions	
DI	Device Identifier – (GS1 UK GTIN 13 used)	AI (01) – Application identifier 01
SN	Serial Number	AI (21) – Application identifier 21
LOT	Lot / Batch Number	AI (10) – Application Identifier 10
	Date of manufacture	AI (11) – Application Identifier 11
UDI	Unique Device Identifier - collective term for DI, SN, LOT & date of manufacture (all contained within machine readable GS1 DataMatrix)	GS1 DataMatrix = 2D Matrix symbols that can carry all GS1 keys and attributes